

Medical Information Technology 2023 Real World Testing Results Report

Expanse/6.1 Release Acute/Ambulatory/Emergency/Oncology Care Settings

Overview

MEDITECH, as an Electronic Health Record (EHR) vendor, is fortunate to collaborate with many of our customers in facilitating the Real World Testing program established by the Office of the National Coordinator (ONC) as introduced with the 21st Century Cures Act. Under the ONC Health IT Certification Program, MEDITECH, as a Health IT developer conducts Real World Testing ensuring validation of patient access, exchange, and use of Electronic Health Information (EHI). Organizations work with us directly in validating the Real World Testing Cures condition of certification, furthering MEDITECH's commitment to interoperability, and advancing health data exchange for our entire customer base.

MEDITECH customers partnered with us in testing and collecting statistical data for Real World Testing results reporting — connecting with organizations quarterly and expediting metric collection in production environments, which supports health data exchange capabilities with related Real World Testing criteria.

This 2023 Real World Testing Result document outlines the data review, demonstrating the interoperability universally of each associated care setting, based on the corresponding Real World Testing plan. Data was aggregated from 243 healthcare organizations, by product line, utilizing existing performance monitoring tools to demonstrate compliance with the conditions of certification. The information captured is metric-based and contains no Protected Health Information (PHI) data. Result reporting instances included verification for data export, transitions of care, electronic prescribing, clinical information reconciliation and incorporation, clinical quality measures, public health interfaces, and Application Programming Interfaces (API).

Products and Certificate Numbers

Product Name(s): Expanse, 6.1

Version Number(s): 2.2, 2.1, 6.15, 6.1

Expanse 2.2 - 2015 Cures Update Certificate Number

MEDITECH Expanse Core HCIS v2.2c (6/30//22) 15.04.04.2931.MEDI.CO.02.1.220630

MEDITECH Expanse Emergency Department Management v2.2c 15.04.04.2931.MEDI.ED.03.1.220630
(06/30/22)

MEDITECH Expanse Ambulatory v2.2c (06/30/22) 15.04.04.2931.2931.02.03.1.220630

MEDITECH Continuity of Care Interface (CCD) v6.1c (06/30/22) 15.04.04.2931.MEDI.61.01.1.220630

MEDITECH Patient and Consumer Health Portal v2.0c (09/19/22) 15.04.04.2931.MEDI.02.01.1.220919

MEDITECH Public Health Interface Transmission to Immunization 15.04.04.2931.MEDI.IR.00.1.171227

Registries v6.1 (12/27/17)

MEDITECH Public Health Interface for Syndromic Surveillance 15.04.04.2931.MEDI.PH.00.1.171226
v6.1 (12/26/17)

MEDITECH Transmission of Reportable Laboratory Test 15.04.04.2931.MEDI.T6.00.1.171226
and Values/Results v6.1 (12/26/17)

MEDITECH Cancer Case Reporting v6.1 (12/26/17) 15.04.04.2931.MEDI.61.00.1.171226

MEDITECH ExpansE Oncology v2.2c (06/30/22) 15.04.04.2931.MEDI.ON.02.1.220630

ExpansE 2.1 - 2015 Cures Update

MEDITECH ExpansE 2.1 Core HCIS v2.1c (06/30/22) 15.04.04.2931.MEDI.CO.01.1.220630

MEDITECH ExpansE 2.1 Emergency Department Management v2.1c (06/30/22) 15.04.04.2931.MEDI.16.02.1.220630

MEDITECH ExpansE 2.1 Ambulatory v2.1c (06/30/22) 15.04.04.2931.2931.16.02.1.220630

MEDITECH Continuity of Care Interface (CCD) v6.1c (06/30/22) 15.04.04.2931.MEDI.61.01.1.220630

MEDITECH Patient and Consumer Health Portal v2.0c (09/19/22) 15.04.04.2931.MEDI.02.01.1.220919

MEDITECH Public Health Interface Transmission to Immunization Registries v6.1 (12/27/17) 15.04.04.2931.MEDI.IR.00.1.171227

MEDITECH Public Health Interface for Syndromic Surveillance v6.1 (12/26/17) 15.04.04.2931.MEDI.PH.00.1.171226

MEDITECH Transmission of Reportable Laboratory Test and Values/Results v6.1 (12/26/17) 15.04.04.2931.MEDI.T6.00.1.171226

MEDITECH Cancer Case Reporting v6.1 (12/26/17) 15.04.04.2931.MEDI.61.00.1.171226

MEDITECH ExpansE 2.1 Oncology v2.1c (06/30/22) 15.04.04.2931.MEDI.ON.02.1.220630

6.1 - 2015 Cures Update

MEDITECH 6.1 Electronic Health Record Core HCIS v6.15c (06/30/22) 15.04.04.2931.MEDI.HC.00.1.171220

MEDITECH 6.1 Emergency Department Management v6.15c (06/30/22) 15.04.04.2931.MEDI.15.00.1.171227

MEDITECH 6.1 Ambulatory Electronic Health Record v6.15c (06/30/22) 15.04.04.2931.MEDI.AM.00.1.171227

MEDITECH Continuity of Care Interface (CCD) v6.1c (06/30/22) 15.04.04.2931.MEDI.61.01.1.220630

MEDITECH Patient and Consumer Health Portal v2.0c (09/19/22) 15.04.04.2931.MEDI.02.01.1.220919

MEDITECH Public Health Interface Transmission to Immunization Registries v6.1 (12/27/17) 15.04.04.2931.MEDI.IR.00.1.171227

MEDITECH Public Health Interface for Syndromic Surveillance v6.1 (12/26/17) 15.04.04.2931.MEDI.PH.00.1.171226

MEDITECH Transmission of Reportable Laboratory Test and Values/Results v6.1 (12/26/17) 15.04.04.2931.MEDI.T6.00.1.171226

MEDITECH Cancer Case Reporting v6.1 (12/26/17) 15.04.04.2931.MEDI.61.00.1.171226

MEDITECH 6.1 Oncology v6.15c (06/30/22) 15.04.04.2931.MEDI.ON.00.1.180503

Care Settings

Real World Testing is demonstrated following typical physician workflow — providing care in Acute, Ambulatory, Emergency Department, or Oncology care settings. Scenarios incorporate Cures Edition certification criteria for testing purposes within the Care Coordination, Clinical Quality Measures, Patient Engagement, Public Health, and Health IT Design and Performance categories.

Changes to Original Plan

The previous testing of 170.315(b)(9) Care plan (6.15 release) has been removed as the Certified Health IT Product List (CHPL) listing has since been retired as a certified product.

The previous testing of Application Programming Interface for (API) §170.315(g)(8) — Application access — data category request has been retired as of 12/31/22 and replaced with §170.315(g)(10) Standardized API for patient and population services. The previous method of quarterly execution of Application Programming Interface via Postman validation for (API) §170.315(g)(7), (g)(9), and now (g)(10) has been modified. This data confirmation has since been updated with a metric-based solution. A sample of Expanse/6.1 customers was evaluated for the successful submission of API requests in a given timeframe by patient identification, multi-patient authorization, and full documentation based on CDA generation and transmission tables.

Testing Methods

Data has been aggregated from a number of healthcare organizations by product line, utilizing existing performance monitoring tools to demonstrate compliance with the conditions of certification. Interfaces have been tested for interoperability, universally of each care setting certified within the CHPL listings for those criteria included within the Conditions and Maintenance of Certification: Real World Testing (170.405). The information captured is metric-based and contains no Protected Health Information (PHI) data.

The following testing methods were utilized to demonstrate real-world interoperability:

- Quarterly review of Management Information System (MIS) interface logs for Expanse/6.1 customers evaluating electronic health exchange (EHI) of Care Coordination, Patient Engagement, and Public Health criteria demonstrating a percentage of messages sent across the related interfaces. A sample of Expanse/6.1 customers was evaluated; the number of accepted messages well exceeds the Promoting Interoperability measurements related to each criteria.
- Quarterly review of the SQL Server Management Studio (SSMS) for a sample of 32 Expanse/6.1 customers was evaluated for Clinical Quality Measures (CQM) and Antimicrobial Use and Resistance (AUR) reporting for the successful submission of Quality Reporting Document Architecture (QRDA) files in a given timeframe.
 - Challenges with AUR/CQM evaluations included timing of customer reviews, reports run, and QRDA submissions throughout the year.
 - The number of CQM reports run and related QRDA submissions well exceed Promoting Interoperability measurements related to each criteria.
- Quarterly execution of Application Programming Interface (API) conformance via customer production rings for each release — Quarterly execution of Application Programming Interface (API) conformance via SQL Server Management Studio (SSMS).
- Quarterly validation via internal Certification environment with synthetic patient data simulating the execution of the creation of data export file(s) and cancer registry reporting for each Expanse/6.1 release.
 - Challenges involved a lack of customer participation resulting in alternate methods being utilized due to non-deployed capabilities in customer production environments with the associated criteria.
 - This test methodology primarily tested the conformance of the implementation.

Measures: Scenarios and Testing Elements: EHI

Sharing of Electronic Health Information - demonstrates MEDITECH's Health IT module conforms to the following certification criteria: § 170.315(b)(1) Transitions of Care, (b)(6) Data Export, and § 170.315(e)(1) View, Download, and Transmit to 3rd party.

The chart below outlines the measures identified to best demonstrate conformance to multiple certification criteria concerning the sharing of Electronic Health Information across the two use cases demonstrated (single patient and population services).

Measure 1 – Sharing EHI	Method
§ 170.315(b)(1) Transitions of care	(i)(A) Send transition of care/referral summaries (i)(B) Receive transition of care/referral summaries
§ 170.315(e)(1) View, download, and transmit	(i)(B)(2) Download ambulatory summary or inpatient summary using CCD Template (i)(B)(3) (Inpatient setting only) Download of transition of care/referral summaries (i)(C)(1) Transmit to third party (i)(C)(2) (Inpatient setting only) Transmit transition of care/referral summaries

Use Case

Sharing of Electronic Health Information Use Case 1 (Single Patient Overview) MEDITECH's fully web-based solution is an integrated component of MEDITECH's enterprise-wide EHR consisting of advanced patient management; at the center of MEDITECH's EHR is a single electronic patient record. This Certified Health IT Module is utilized when documentation needs to be coordinated between providers and patients both internally and externally within a healthcare organization.

- MEDITECH demonstrates that both a limited and full set of data, as required in the United States Core Data for Interoperability (USCDiv1) standard, can be sent and received for Transition of Care (TOC) documentation for a single patient.
- The data can be shared externally using Edge protocol technology (Direct, SMTP email), exported, and shared directly with the patient through MEDITECH's Patient Portal. This functionality provides the ability to view, download, and transmit data.
- TOC summaries provide essential clinical information for the receiving care team and help organize final clinical and administrative activities for the transferring care team. MEDITECH's enterprise-wide EHR ensures the timely availability of patient information within the Inpatient, Ambulatory, Emergency Department, and Oncology care settings.

United States Core Data for Interoperability (USCDiv1) standard can be sent and received on documentation for a single patient. The Inpatient, Ambulatory, Emergency Department, and Oncology settings include two capabilities for conformance: (1) Sending transition of care/referral summaries and (2) Receiving transition of care referral summaries, including XDM processing.

- The Patient and Consumer Health Portal is a fully-integrated component of MEDITECH's IT module.
- Seamless exchange of information ensures patients and staff alike have timely access to accurate and timely data across care settings.
- Metrics provide details on the types of transmissions deployed and the frequency of usage.

Test Methodology

MEDITECH reporting logs were utilized to monitor Management Information System (MIS) interfaces to determine the frequency and the transport workings used by providers for sending and receiving transitions of care and downloading or transmitting data via MEDITECH's Patient Portal.

- Logs obtained during real world testing were de-identified and used for analysis in several areas to validate the proper operation of the transport system and input for the calculation of the metric on the specific types of transport functionality utilized.
- The data metrics associated with criteria in these scenarios confirm the ability to create, receive, and properly consume interoperable documents using a common content and transport standard (e.g., Consolidated Clinical Document Architecture (C-CDA) that includes key health data — accessible and available for exchange).

Justification

The Inpatient, Ambulatory, Emergency Department, and Oncology settings include two capabilities for conformance: (1) Sending transition of care/referral summaries and (2) Receiving transition of care referral summaries. Transitions of care (TOC) documents are shared using connection protocols (e.g., SMTP, Direct) while other data may be shared through MEDITECH's Patient Portal using downloads and encrypted or unencrypted transmissions.

- The Patient and Consumer Health Portal is a fully-integrated component of MEDITECH's IT module.
- Seamless exchange of information ensures patients and staff alike have timely access to accurate and timely data across care settings.
- Quarterly metrics provided details on the types of transmissions deployed and the frequency of usage.

Final Outcome(s):


A total number of summary of care messages were generated for each transition of care request either receiving or sending information upon receipt of a transition. The functionality of incorporating the summary of care information provides a seamless transition into or out of the MEDITECH EHR. Providers and patients (or their authorized representatives) share data using the transmission functionality provided for Medicare Eligible Hospitals (EHs), Critical Access Hospitals (CAHs), and Medicaid Eligible Professionals (EPs) to meet or surpass the requirements of Promoting Interoperability programs related to Coordination of Care. Success and error rates were tracked and trended over time.

Measurement/Metric Findings:


In reviewing reports for Electronic Health Exchange (EHI), the number of accepted messages well exceeded Promoting Interoperability measurements related to each criteria. Result totals included the following number of accepted messages for all related interface types with no challenges encountered:

- § 170.315(b)(1) Transitions of care 33,618,456 total transactions demonstrating transmitting a set of documents and associated metadata for a combined 98.83% success rate
- § 170.315(e)(1) View, download, and transmit - 1,906,205 patient portal transactions including medication renewal requests, allergy, and full health summary views related to VDT criteria were populated for a combined 100.00% success rate

Transitions of Care: Success Rate by Platform

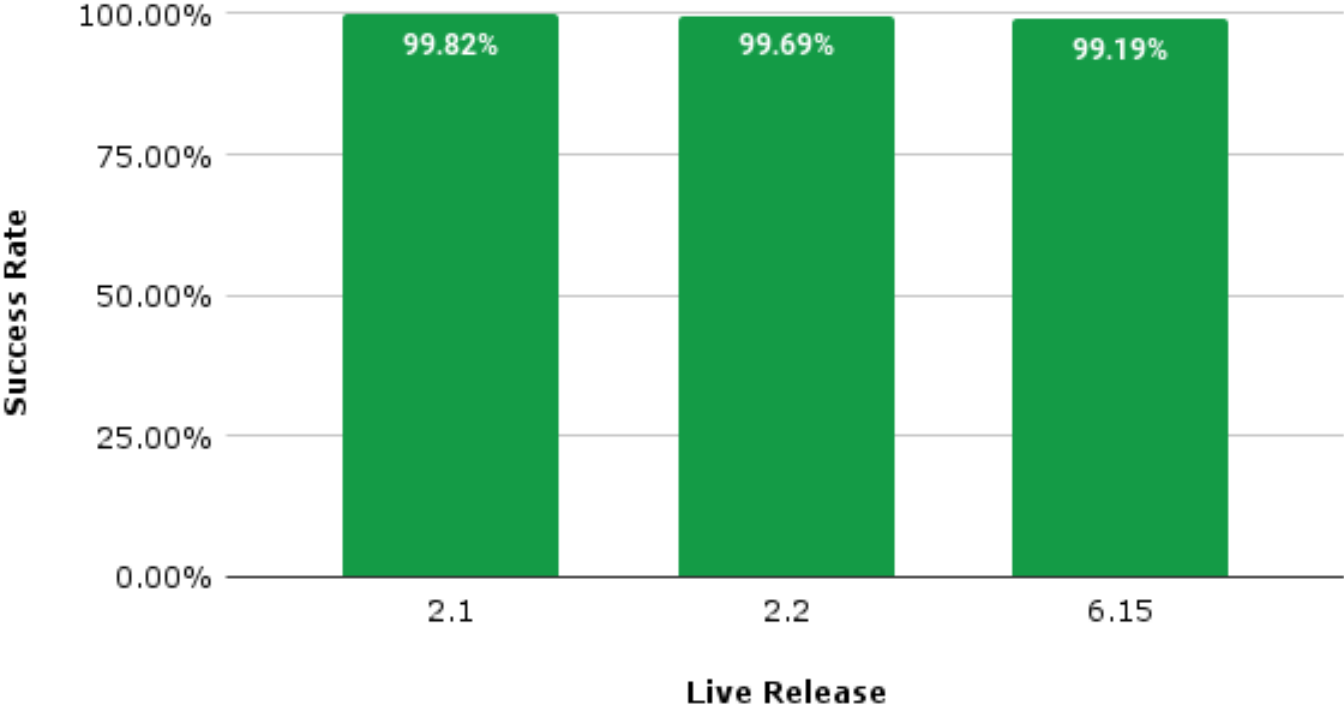

View, Download, Transmit: Success Rate by Platform

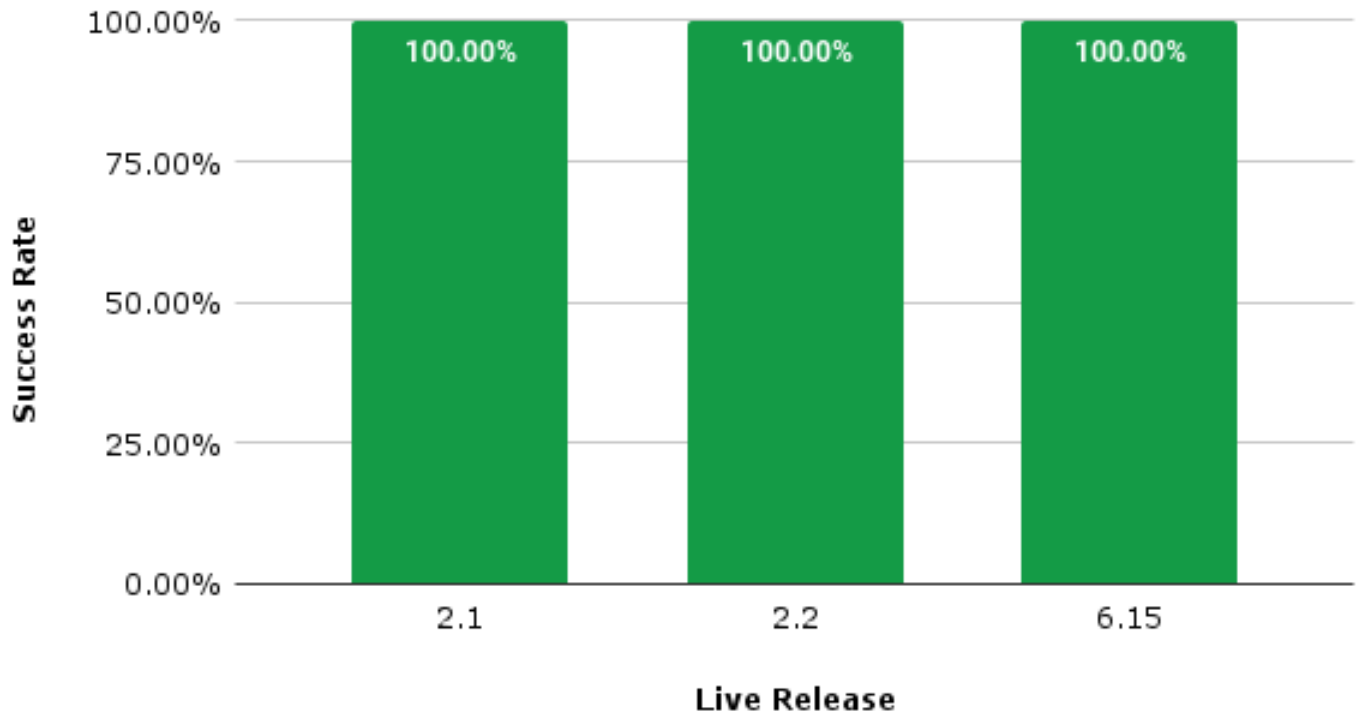

Measure 2 – Patient Export	Method
(b)(6) Data Export	(6)(ii) Create export file (6)(iii)(A) real-time export; export based upon a relative date; and export based upon a specific date. (6)(iii)(B) Execute export

Test Methodology

MEDITECH reporting logs were utilized to monitor Management Information System (MIS) interfaces to ensure the export function is operating properly and to determine the frequency of use. Logs obtained during Real World Testing were de-identified and utilized for analysis in several areas to validate the proper operation of the export. This test methodology primarily tests the conformance of the implementation.

Justification

The export of data associated with a patient population is an additional way to share health information with external organizations. The intent is to provide data research to analyze specific trends in the patient population, export of which is only available to authorized users. This provided a metric on the use of the export of data for a patient population associated with MEDITECH's Health IT Module.

Final Outcomes


The Internal system logs were reviewed to ensure the export function is operating properly and to determine the frequency of use. Logs obtained during Real World Testing were de-identified and utilized for analysis in several areas to validate the proper operation of the export. This test methodology primarily tests the conformance of the implementation. Transmissions were tracked and analyzed over time.

Measurement/Metric Findings

In reviewing reports for Electronic Health Exchange (EHI) with Data Export, **the number of accepted messages well exceeds** Promoting Interoperability measurements related to the criteria. Result totals included the following accepted messages for the related interface type with no challenges encountered:

- (b)(6) Data Export Export 42,432,838 XML files with the Data Export routine message type for a combined 99.64% success rate

Data Export: Success Rate by Platform

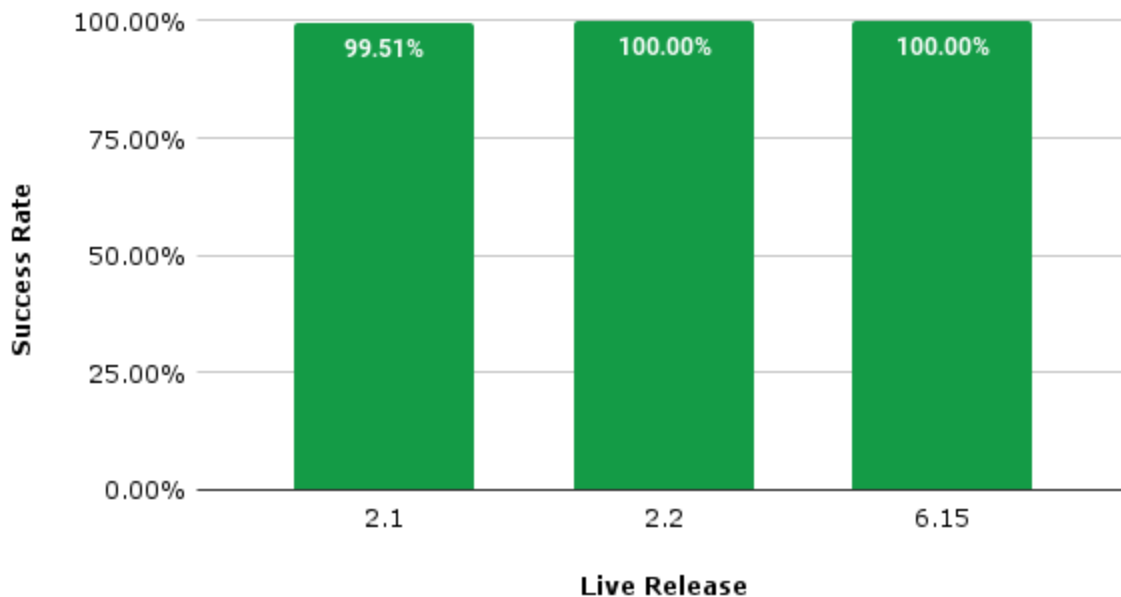

Measures: Scenarios and Testing Elements: Clinical Information Reconciliation and Incorporation (CIRI)

The chart below outlines the measures that have been identified to best demonstrate conformance to Clinical Information Reconciliation and Incorporation (CIRI) certification criteria concerning the ability to maintain and review accurate medication, allergy, and problem lists for a patient — enabling clinicians to make informed care decisions during office visits.

Clinical Information Reconciliation and Incorporation	Method
§170.315(b)(2) Clinical Information Reconciliation and Incorporation	(b)(2)(ii) transition of care summary/referral summary Consolidated-Clinical Document Architecture (C-CDA) document can be properly matched to a patient in the

	<p>Health IT Module (automatically or manually). (b)(2)(iii)(B) user creates a single, reconciled list using the data reviewed from the multiple medications, problems, or medication allergies (b)(2)(iii)(D) user accepts the reconciled list</p>
--	---

Use Case

MEDITECH demonstrates (CIRI) by comparing information from the MEDITECH system with information from external sources, such as discussions with the patient or a CCD to ensure the data on the patient's chart is up to date. An inbound CCD is received for patients and any unmatched CCD medications, allergies, or problems are displayed. Metrics provided details on the number of reconciliations deployed and the frequency of usage.

Test Methodology

MEDITECH reporting logs were utilized to monitor Management Information System (MIS) interfaces to capture percentages for the Support Electronic Referral Loops by Receiving and Incorporating Health Information (Receive and Reconcile) measures. Variables capture the reconciliation percentage of imported problems, medications, or allergies. Logs obtained during Real World Testing were de-identified and used for analysis in several areas to validate the proper operation of (CIRI) transactions. The data metrics associated with the criteria in the above scenario confirm the ability of customers to perform accurate clinical information reconciliation.

Justification

As part of the Real World Testing requirements for §170.315(b)(2) Clinical Information Reconciliation and Incorporation (CIRI), MEDITECH demonstrates that external medications, allergies, and problems are available for reconciliation in order to confirm all current data. MEDITECH’s enterprise-wide EHR ensures the ongoing capabilities in reconciling patient information within the Inpatient, Ambulatory, Emergency Department, and Oncology care settings.

Final Outcome(s):


A total number of transitions or referrals receiving and incorporating Health Information (external medications, allergies, and problems) by performing a clinical information reconciliation were captured over a period for the Real World Test population of patients. This data exchange allows EHs/CAHs and Medicaid EPs to meet or surpass requirements of the Health Information Exchange objective Measure 3 - Clinical Information Reconciliation for threshold-based reporting and the Support Electronic Referral Loops by Receiving and Incorporating Health Information measure for performance-based reporting. Success and error rates were tracked and trended over time.

Measurement/Metric Findings:

A review of reports for Electronic Health Exchange (EHI) with CIRI found **the number of accepted messages well exceeds** Promoting Interoperability measurements related to the criteria. Result totals included the following accepted messages for the interface type with no challenges encountered:

- §170.315(b)(2) Clinical Information Reconciliation and Incorporation - 15,368,481 messages for Retrieve Document Set files with a combined 99.99% success rate

Clinical Information Reconciliation and Incorporation (CIRI): Success Rate by Platform

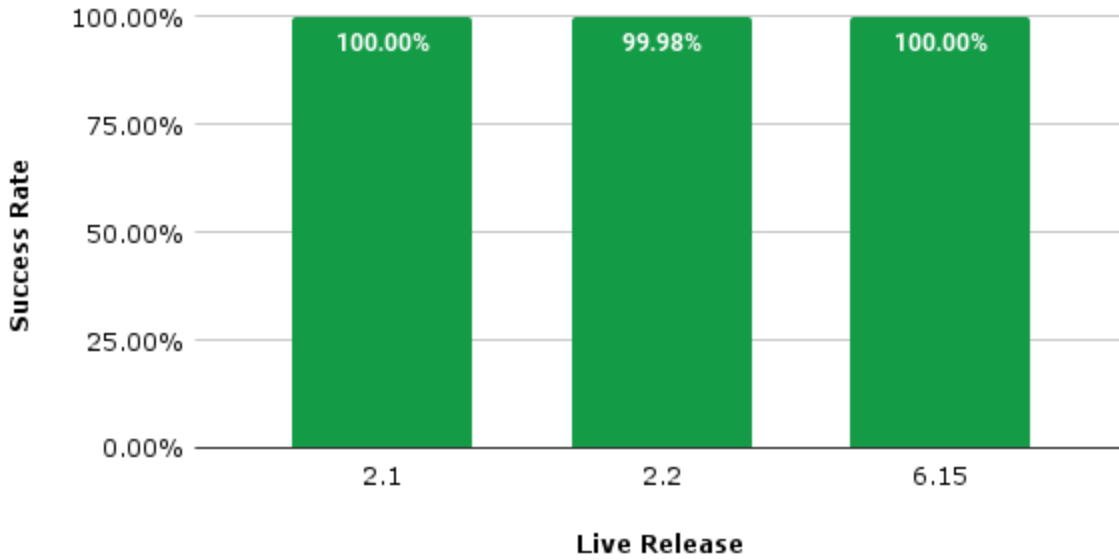

Measures: Scenarios and Testing Elements: Electronic Prescribing

As part of the Real World Testing requirements for §170.315(b)(3) Electronic Prescribing, MEDITECH demonstrates that an authorized user can be enabled to perform required prescription-related transactions in accordance with the standard. MEDITECH enables Electronic Prescribing and Order Communications from a single, central location. This Certified Health IT module is utilized when clinicians need to enter individual orders or multi-disciplinary order sets for prescription orders. The eRX orders are communicated in real-time to the receiving ancillary department's desktop, and clinicians can easily cancel, edit, renew, repeat, or hold orders at any time.

The chart below outlines the measures that have been identified to best demonstrate conformance to Electronic Prescribing (eRX) certification criteria concerning the ability to perform prescription-related transactions. This functionality includes creating new prescriptions, changing prescriptions, transmitting and receiving medication-associated diagnoses, and reasons for each prescription transaction.

Electronic Prescribing	Method
§170.315(b)(3) Electronic Prescribing	(b)(3)(ii)(A) send and receive specified prescription transactions electronically (all eRX transaction types) (b)(3)(ii) (C) send and receive the reason for the prescription (all eRX transaction types)

Use Case

MEDITECH's eRX capabilities are offered in collaboration with DrFirst. Functionality supported includes the ability to electronically submit prescriptions to outpatient pharmacies, review medication claim histories, electronically query a patient's prescription drug plan to ensure eligibility, and check the insurance formulary for covered medications.

Test Methodology

Reports and interface logs were reviewed to determine the frequency of transaction transmissions, outbound requests, and inbound responses. Logs obtained during Real World Testing were de-identified and used for analysis in several areas to validate the proper operation of eRX transactions. The metrics associated with the criteria in the above scenario confirm the ability of customers to generate and transmit permissible prescriptions electronically.

Justification

The Inpatient, Ambulatory, Emergency Department, and Oncology settings include the following capabilities for conformance: receiving and processing a number of electronic transactions for new prescriptions; requests to change, cancel, or refill prescriptions; and Medication History Information requests. Metrics provide details on the types of transactions deployed and the frequency of usage.

Final Outcome(s):


Transaction types reconcile the corresponding number of new prescriptions; requests to change, cancel, or refill prescriptions; and Medication History Information requests. A total number of messages were generated for each eRX request either receiving or sending prescriptions for the Real World Test population of patients. Authorized users generate and transmit permissible discharge prescriptions electronically for EHs/CAHs and Medicaid EPs to meet or surpass (eRX) requirements for Promoting Interoperability criteria. Success and error rates were tracked and trended over time.

Measurement/Metric Findings:

A review of reports for Electronic Prescribing found **the number of accepted messages well exceeds** Promoting Interoperability measurements related to the criteria. Result totals included the following accepted messages for the interface type with no challenges encountered:

- §170.315(b)(3) Electronic Prescribing - 4,034,065 total messages for eRX categories with a combined 99.91% success rate

Electronic Prescribing: Success Rate by Platform

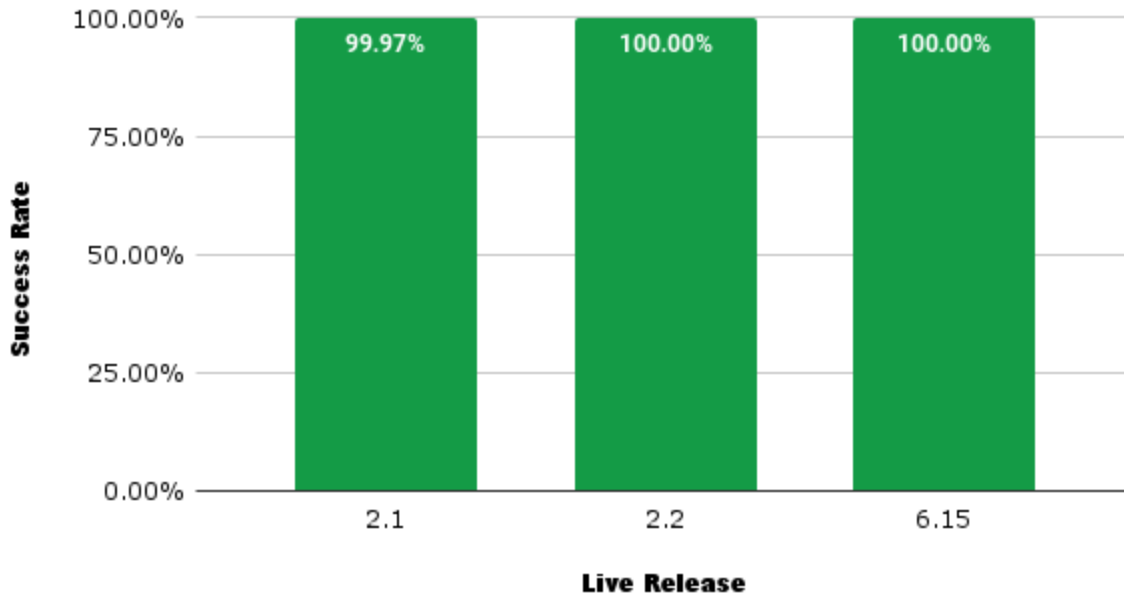

Measures: Scenarios and Testing Elements: Clinical Quality Measures

This Real World Testing scenario demonstrates that MEDITECH's Health IT Module conforms to the following certification criteria: §170.315(c)(1) Clinical Quality Measures - Record and Export, §170.315(c)(2) Clinical Quality Measures - Import and Calculate, and §170.315(c)(3) Clinical Quality Measures – Report.

The chart below outlines the measures that have been identified to best demonstrate conformance to multiple certification criteria to capture the reporting and execution of QRDA files.

Clinical Quality Measures	Method
§170.315(c)(1) Clinical Quality Measures - Record and Export	(c)(1)(i) user demonstrates that they can record the specified data needed for each of the certified CQMs - Record Entry - Record Batch Entry (c)(1)(ii) user can export a file at any time the user chooses and without subsequent developer assistance.
§170.315(c)(2) Clinical Quality Measures - Import and Calculate	(c)(2)(i) user can execute the import capability described in (c)(2)(i) any time the user chooses and without subsequent developer assistance to operate. (c)(2)(ii) user calculates the aggregate reports for each of the CQMs for which they are seeking certification, based upon the imported and de-duplicated data set. The Health IT Module submits an aggregate report for each of the CQMs to be certified.

<p>§170.315(c)(3) Clinical Quality Measures - Report</p>	<p>(c)(3)(i) (1) user can generate an aggregate report (QRDA Category III) (2) user can generate a de-duplicated archive of patient documents in the QRDA Category I format of the clinical quality measures calculated in the Execute test (§ 170.315(c) (3) The health IT developer submits the quality measurement data file consisting of the data created by the generation of the QRDA Category III aggregate report(s) and the de-duplicated QRDA Category I report(s) for verification.</p>
--	---

Use Case

MEDITECH reporting is utilized to demonstrate that a user can export a QRDA Category I file(s) for a single patient at any time the user chooses (on-demand) and a list of SQL reports templates is available for customers, corresponding to each required Clinical Quality Measure report specifications and the QRDA Category 1 updates necessary for electronic reporting.

Test Methodology

Reporting logs were reviewed to capture the number of clinical quality measure percentages over a period of time based on the specific measure being qualified. Logs obtained during Real World Testing were de-identified and used for analysis in several areas to validate the proper operation of QRDA transactions. The data metrics associated with the criteria in the above scenario confirm the ability of customers to facilitate accurate Clinical Quality Measure reporting.

Justification

MEDITECH’s ARRA Report Manager is a web-based solution for executing MEDITECH’s Meaningful Use reports, including variables that capture reporting and execution of QRDA files. The auditing functionality allows for an audit trail of the report execution and results to be saved in audit tables to be used for attestation runs. Metrics provided details on the number of transactions saved for attestation and the frequency of usage.

Final Outcome(s):

EHS/CAHs and Medicaid EPs meet or surpass requirements by attesting to measures. A total number of saved attestations are captured for a specific reporting period for the Real World Test population of patients and were tracked and trended over time.

Measurement/Metric Findings:

A review of reports for Clinical Quality Measures (CQM) reporting for the successful submission of Quality Reporting Document Architecture (QRDA) files — CQM reports run and the total number of QRDA submissions for both Eligible Hospitals and Eligible Clinicians are evaluated quarterly. Result totals included the following statistics for the criteria:

- §170.315(c)(1) Clinical Quality Measures - Record and Export
- §170.315(c)(2) Clinical Quality Measures - Import and Calculate
- §170.315(c)(3) Clinical Quality Measures - Report

Clinical Quality Measures were evaluated for a sample of Expanse/6.1 customers quarterly with 650 combined reports compiled. Additionally, 215 QRDA files were submitted and accepted for CQM/AUR reporting attestation in this cross-check for Promoting Interoperability measurements. Findings included measures for both Eligible Hospitals and Eligible Providers/Clinicians.

Challenges with CQM evaluations included timing of customer reviews, reports run, and QRDA submissions throughout the year. The number of CQM reports run and related QRDA submissions well exceed Promoting Interoperability measurements related to each criteria.

Measures: Scenarios and Testing Elements: Public Health Interfaces

The Real World Testing scenario below demonstrates that MEDITECH’s Health IT module conforms to the following certification criteria: §170.315(f)(1) Transmission to Immunization Registries, §170.315(f)(2) Transmission to Public Health Agencies - Syndromic Surveillance, and §170.315(f)(3) Transmission to Public Health Agencies - Reportable Laboratory Tests and Value/Results.

The chart below outlines the measures that have been identified to best demonstrate conformance to multiple certification criteria concerning the sharing of registry data as demonstrated through the use case for population services.

Public Health Interfaces	Method
§170.315(f)(1) Transmission to Immunization Registries	(f)(1)(i) (1) generate the indicated HL7 v2.5.1 Z22 VXU immunization information message, (2) consume the associated acknowledgment message, (3) maintain historical vaccine records (f)(1)(ii) receive HL7 evaluated immunization history and forecast HL7 v2.5.1 Z42 RSP or HL7 v2.5.1 Z33 RSP response messages
§170.315(f)(2) Transmission to Public Health Agencies - Syndromic Surveillance	(f)(2) (2) generate the indicated HL7 v2.5.1 ADT message
§170.315(f)(3) Transmission to Public Health Agencies - Reportable Laboratory Tests and Value/Results	(f)(3)(i) create Reportable Lab content and generate ELR message

Use Case

At the foundation of any effective population management solution is data, and MEDITECH’s EHR brings it all together through reporting solutions in capturing public health criteria. Our EHR aggregates data across the continuum of care — from customer hospitals, physician practices, emergency departments, and long-term care facilities. MEDITECH’s Certified Health IT module provides functionality to track and store patient immunization information electronically, ensure hospitals possess the ability to report threat and outbreak information to public health agencies with Syndromic Surveillance data, as well as reportable condition functionality where specific reportable laboratory tests and results are defined.

Test Methodology

MEDITECH reporting logs were utilized to monitor Management Information System (MIS) interfaces to capture percentages to ensure the transmissions are operating properly and to determine the frequency of use. Logs obtained during Real World Testing were de-identified and utilized for analysis in several areas to validate the proper operation of the Public Health interfaces. This test methodology primarily tests the conformance of the Implementation.

Justification

The transmission of Public Health data associated with a patient population using interface functionality provides data research to analyze specific trends in the patient population. With intuitive, web-based interfaces, MEDITECH's Public Health & Clinical Data Exchange functionality within the Inpatient, Ambulatory, and Emergency Department settings includes seamless and active engagement with public health agencies or clinical data registries to submit electronic public health data for conformance to this combined criteria. Interface messages provide metrics on the use and frequency of transmissions to state agencies for immunizations, syndromic surveillance, and reportable laboratory tests, value/results for a patient population associated with MEDITECH's Health IT Module.

Final Outcome(s):


Public Health messages are processed and received via the interfaces used by the healthcare organization. Eligible hospitals or professionals are in active engagement with a public health agency using functionality provided in order to submit electronic public health data for EHS/CAHs and Medicaid EPs to meet or surpass requirements of Promoting Interoperability programs related to Public Health and Clinical Data Exchange objectives. Success and errors in transmission were tracked and analyzed over time.

Measurement/Metric Findings:

A review of sent messages for each public health interface was reviewed for result totals included in the following statistics for the criteria with no challenges encountered:


- §170.315(f)(1) Transmission to Immunization Registries - Immunization Query and Response 75,967,541 messages with a combined 99.78% success rate

Transmission to Immunization Registries - Immunization Query and Response: Success Rate by Platform

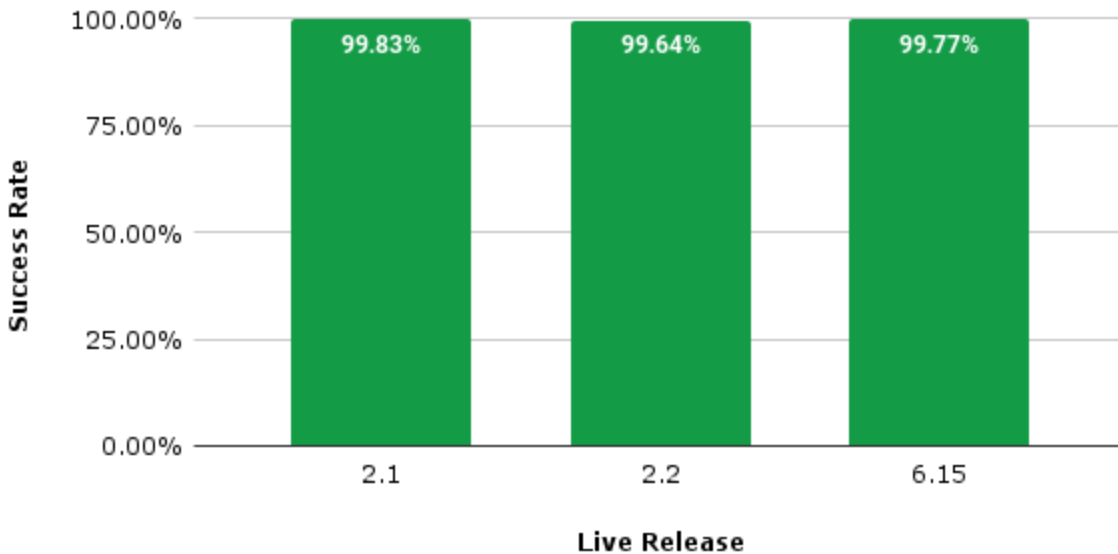


- §170.315(f)(2) Transmission to Public Health Agencies - Syndromic Surveillance Admission, Discharge, Transfer (Inbound and Outbound) 184,366,337 messages with a 99.96% combined success rate

Transmission to Public Health Agencies - Syndromic Surveillance: Success Rate by Platform

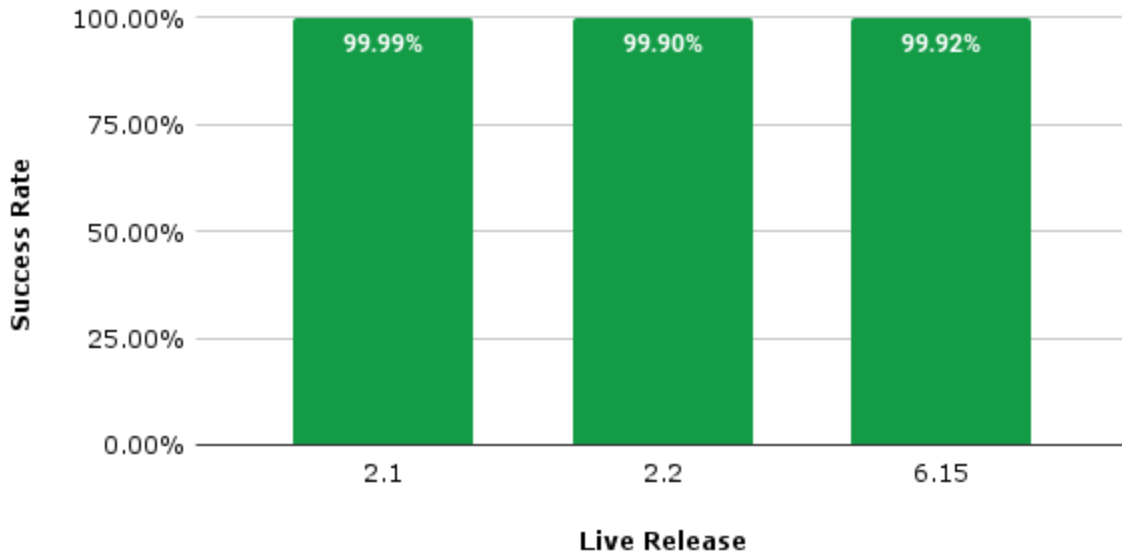

- §170.315(f)(3) Transmission to Public Health Agencies - Reportable Laboratory Tests and Value/Results (Inbound and Outbound) 129,141,869 messages with a 100.00% combined success rate

Transmission to Public Health Agencies - Reportable Laboratory Tests and Value Results: Success Rate by Platform

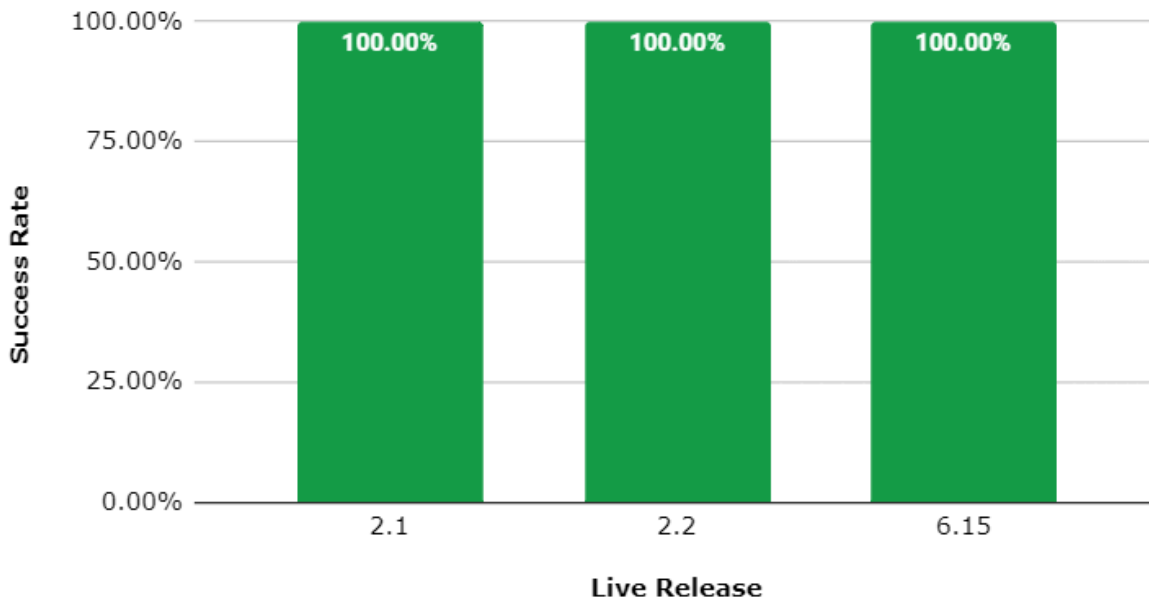

Measures: Scenarios and Testing Elements: Cancer Registries

The chart below outlines the measures that have been identified to best demonstrate conformance to §170.315(f)(4) Transmission to Cancer Registries criteria concerning the sharing of registry data as demonstrated through the use case for population services.

Public Health Interfaces: Cancer Case Reporting	Method
§170.315(f)(4) Transmission to Cancer Registries	(f)(4)(i) (2) create cancer case document, Reporting to Public Health Cancer Registries

Use Case

Cancer Event Reporting is incorporated into MEDITECH's workflow allowing organizations to use functionality in meeting the MIPS criteria established by the Medicare Access and CHIP Reauthorization Act of 2015 (MACRA) for Public Health Registry Reporting. MEDITECH's Cancer Registry interface generates outbound messages to meet this measure.

Test Methodology

In order to effectively monitor cancer conditions and meet MIPS requirements, organizations must capture a variety of data elements that the system uses to populate cancer event reports. These data elements include patient demographics, provider and organization information, cancer diagnosis and details, laboratory and pathology results, and medication information. MEDITECH demonstrates the capability of generating a cancer event report when a testing patient is diagnosed with an ICD code recognized by the Centers for Disease Control (CDC) as a cancer condition.

Justification

As part of the Real World Testing requirements for § 170.315(f)(4), MEDITECH demonstrates Reporting to Public Health Cancer Registries via validation reports following standard workflow within dedicated internal platforms for Acute, Oncology, and Ambulatory settings.

Final Outcome(s):

Using a dedicated internal platform, testing confirmed Cancer Case trigger routines respond to and generate a corresponding cancer event report. Visual inspection of success rates with MEDITECH's interface message generator was captured to demonstrate the capability with outbound messages for Cancer Case reporting. Negative testing to confirm diagnosis codes not matching the Cancer Case trigger was also validated quarterly.

Measurement/Metric Findings:

A review of sent messages for each cancer case event was reviewed for result totals included in the following statistics for the criteria with no challenges encountered:

- §170.315(f)(4) Transmission to Cancer Registries - Results included 100% success rates with 36 accepted Cancer Event messages for combined releases quarterly.

Cancer Case Reporting Sample Q4 2023 - Expanse 2.2 Validation

cert22x-web01.meditech.com/cert22x/s0002456607038725/

NIST Cancer Case Add Addendum Save

Principal Meditech Mt Contributors Last Saved at 11/27/23 11:57 am

View Document Office Procedures Departure

Smith, Jane
 59, F · 08/30/1964
 MRN# MR00002735

REG AM
 AMB

Arrived
 REG AM
 AMB

Visit Date: 11/27/23

Resus Status Not Addressed
 No Hx Avail

Search Patient's Chart

Special Indicators
 No Data to Display

Vital Signs
 No Data to Display

Home Meds
 No Data to Display

Allergies

Allergies					
Allergy/AdvReac	Type	Severity	Reaction	Status	Date / Time
amoxicillin	Allergy	Intermediate	Hives	Verified	06/13/23 14:08

Visit Care Team: Meditech Mt
 Role: Attending Provider
 Specialty: Internal Medicine
 Phone: 555-789-9090

Provider Type: Staff Physician

Assessment & Plan
Assessment & Plan
 (1) Malignant neoplasm of upper lip:
 Status: Acute
 Comment:
 Attaching cancer case problem to document.
 Code(s):
 C00.0 - Malignant neoplasm of external upper lip
 SNOMED Code(s): 363348004
 Category: Medical

cert22x-web01.meditech.com/cert22x/s0002456607038725/

Interface Manager (CERT22XN.US)

Interface: CDA Compile Service: Generator (ARCHIVE.ACR) Messages
 Name: CDA Compile Name: Archive Cancer CDA
 Direction: SEND Status: RUNNING Newest: 2320436
 Oldest: 2320434

Status Messages Backlogs

✓	Interface/Service	I/O	Name	State	Msgs Fltrd	Job
<input type="checkbox"/>	AMBLAB	I/O	Ambulatory Inbound Lab Results	On/Off		
<input type="checkbox"/>	CDA Compile	I/O	CDA Compile	On		
<input type="checkbox"/>	Delivery	I	CDA Compile	On		
<input checked="" type="checkbox"/>	Generator	O	Archive Cancer CDA	On		
<input checked="" type="checkbox"/>	Generator	O	Archive CDA	On		
<input type="checkbox"/>	CDA ConsumerBH	I/O	CDA Consumer BH	On/Off		
<input type="checkbox"/>	CDA PatIdMgrBH	I/O	CDA Patient Identity Manager BH	On/Off		
<input type="checkbox"/>	CDA SupplierBH	I/O	CDA Supplier BH	On/Off		
<input type="checkbox"/>	DIR ETT IN	I	ETT XDR Inbound	Off		
<input type="checkbox"/>	DIR ETT OUT	I/O	ETT XDR Outbound	On		
<input type="checkbox"/>	DIR XDR IN	I	Direct XDR Inbound	Off		
<input type="checkbox"/>	DIR XDR OUT	I/O	Direct XDR Outbound	On		

Outbound Messages - Generator ARCHIVE.ACR

✓	Message	Date/Time	Source	Source ID	Message Type	Status
<input type="checkbox"/>	2320436	11/27 1158	MRI.STD	ARCHIVE.ACR	ARCHIVE.ACR	SENT
<input type="checkbox"/>	2320435	11/27 1158	MRI.STD	ARCHIVE.ACR	ARCHIVE.ACR	SENT
<input type="checkbox"/>	2320434	11/27 1158	MRI.STD	ARCHIVE.ACR	ARCHIVE.ACR	SENT

Measures: Scenarios and Testing Elements: Antimicrobial Use and Resistance Reporting

The chart below outlines the measures that have been identified to best demonstrate conformance to §170.315(f)(6) Transmission to Public Health Agencies - Antimicrobial Use and Resistance Reporting criteria concerning the sharing of registry data as demonstrated through the use case for population services.

Public Health Interfaces: AUR Reporting	Method
§170.315(f)(6) Transmission to Public Health Agencies - Antimicrobial Use and Resistance Reporting	(f)(6) (1) Health IT Module creates Antimicrobial use and resistance reporting information Antimicrobial Resistance Option Report (Numerator) Antimicrobial Resistance Option (ARO) Summary Report (Denominator) Antimicrobial Use (AUP) Summary Report (Numerator and Denominator)

Use Case

MEDITECH conforms to the Centers for Disease Control (CDC) specifications for Antimicrobial Use and Resistance Reporting and provides reporting related to generating electronic Microbiology antimicrobial resistance and antibiotic administration reports for transmission to the National Healthcare Safety Network (NHSN). Measures that have been identified to best demonstrate conformance to the AUR reporting certification criteria include report functionality in success percentages for related Promoting Interoperability (PI) Objective measures.

Test Methodology

Reporting logs were reviewed to capture the number of CDA files saved for submission over a period of time. Logs obtained during Real World Testing were de-identified and used for analysis in several areas to validate the execution of Antimicrobial Use and Resistance data. The metrics associated with the criteria in the above scenario confirm the ability of customers to facilitate the export of CDA XML files for accurate AUR reporting.

Justification

MEDITECH reporting capabilities provide a web-based solution for executing MEDITECH's meaningful use reports. AUR reporting includes variables that capture Numerator/Denominator values to assist customers in successfully submitting data in order to receive confirmation of compliance from NHSN. The auditing functionality allows for a history of the report execution and results to be saved in audit tables and used for attestation purposes.

Final Outcome(s):

Authorized users generate electronic Microbiology antimicrobial resistance and antibiotic administration reports for transmission to the National Healthcare Safety Network for EHs/CAHs and Medicaid EPs to meet or surpass requirements related to Public Health and Clinical Data Exchange objectives. A total number of saved CDA XML files are captured for a specific reporting period for the Real World Test population of patients and tracked and trended over time.

Measurement/Metric Findings:

A review of reports for Antimicrobial Use and Resistance data for the successful submission of Quality Reporting Document Architecture (QRDA) files was evaluated for a sample of Expanse/6.1 customers — AUR reports run and a total number of QRDA submissions was evaluated quarterly. Result totals included the following statistics for the criteria:

➤ §§170.315(f)(6) Transmission to Public Health Agencies - Antimicrobial Use and Resistance Reporting

Logs were evaluated for a sample of Expansive/6.1 customers quarterly with 70 reports compiled. Additionally, 56 QRDA files were submitted and accepted for AUR reporting attestation in this cross-check for Promoting Interoperability measurements.

Challenges with AUR evaluations included timing of customer reviews, reports run, and QRDA submissions throughout the year. **The number of reports run and related QRDA submissions well exceeds** Promoting Interoperability measurements related to the criteria.

Measures: Scenarios and Testing Elements: Application Access

The Real World Testing scenario below demonstrates that MEDITECH’s Health IT module conforms to the following certification criteria: §170.315(g)(7) Application Access - Patient Selection, §170.315(g)(9) Application Access - All Data Request, and §170.315(g)(10) Application Access - Standardized API for Patient and Population Services.

The chart below outlines the measures that have been identified to best demonstrate conformance to multiple certification criteria to validate Application Programming Interface (API) interoperability-specific application requests and responses.

Public Health Interfaces: Application Access	Method
§170.315(g)(7) Application Access - Patient Selection	The health IT developer submits their self-declaration to the ONC-ATL.
§170.315(g)(9) Application Access - All Data Request	(g)(9)(i)(A) (2) user demonstrates that the API responds to and returns all data from the USCDI (g)(9)(i)(B) API functions return data to the developer-identified requesting application for a specific date that the requesting application identifies.
§170.315(g)(10) Application Access - Standardized API for Patient and Population Services	(g)(10)(i), (ii) Demonstrate Single Patient API (g)(10)(i), (ii), (iv) Demonstrate Multi-Patient Authorization and API

Use Case

Interoperability Services (IOPS), an Application Programming Interface (API) platform installed alongside the RESTful API Infrastructure, provides the MEDITECH EHR with next-generation interoperability capabilities. The platform runs interoperability-specific applications (collections of APIs) — enabling the MEDITECH EHR to take advantage of more advanced features and integrations. The MEDITECH API platform is an extension of the MEDITECH Health Care Information System (HCIS) which enables client applications to interact with MEDITECH’s databases. Reporting logs track the register of API User clients with the MEDITECH API platform in order to demonstrate the facilitation of Application Access requests for all related criteria.

Test Methodology

Reporting logs were reviewed to capture the number of Application Access requests for patient selection, category, and population requests over a period of time. Logs obtained during Real World Testing were de-identified and used for analysis in several areas to validate the execution of APIs. This test methodology primarily tests the conformance of the implementation.

Justification

MEDITECH remains at the forefront of the interoperability movement. As a contributing member of the CommonWell Health Alliance and a collaborator in Argonaut's FHIR Project, we are committed to increasing our customers' data exchange avenues. Reporting logs reflect the number of successful transactions wherein one or more API routines respond to and return the full set of data for each data category from the USCDI for the unique patient identified by the ID or token.

Final Outcome(s):

Reporting logs reflect the number of patient access (g7), full dataset (g9), and single/multiple patient (g10) requests returning full sets of data for each data category from the USCDI for the unique patient identified by the ID or token. Visual inspection of successful metrics was tracked and analyzed.

Measurement/Metric Findings:

A review of reports for Application Access data for the successful capture of API collections was evaluated for a sample of Expanse/6.1 customers (combined annual totals):

- §170.315(g)(7) Application Access - Patient Selection - patient identifier 4,509,470 (total # of patient events for the given ImplementationID)
- §170.315(g)(9) Application Access - All Data Request 724,503 (total # of events for the given ImplementationID specifically for (CDA))
- §170.315(g)(10) Application Access - Standardized API for Patient and Population Services 163,964 (total # of Globally Unique Identifiers (GUID) with events in more than 1 category for the given ImplementationID)

Related Criteria/Relied-Upon Software	
Criteria	Relied-Upon Software
§170.315(b)(3) Electronic Prescribing	For Ambulatory and Emergency Department Management <ul style="list-style-type: none">● MEDITECH Expanse 2.2 Core HCIS (Version v2.2c) OR● MEDITECH Expanse 2.1 Core HCIS (Version v2.1c) OR● MEDITECH 6.1 Electronic Health Record Core HCIS (Version v6.15c) AND <ul style="list-style-type: none">● DrFirst Rcopia (DrFirst) AND● EPCS Gold (DrFirst) AND

	<ul style="list-style-type: none"> ● First Databank AND ● Medi-Span (Walters Kluwer)
§170.315(b)(6) Data Export	<ul style="list-style-type: none"> ● MEDITECH Continuity of Care Interface (CCD) (Version v6.1c)
<p>§170.315(c)(1) Clinical Quality Measures - Record and Export</p> <p>§170.315(c)(2): Clinical Quality Measures - Import and Calculate</p> <p>§170.315(c)(3): Clinical Quality Measures - Report</p>	<p>For Ambulatory, Emergency Department Management, and Oncology</p> <ul style="list-style-type: none"> ● MEDITECH Expanse 2.2 Core HCIS (Version v2.2c) OR ● MEDITECH Expanse 2.1 Core HCIS (Version v2.1c) OR ● MEDITECH Expanse 2.1 Core HCIS (Version v2.1c) OR ● MEDITECH 6.1 Electronic Health Record Core HCIS (Version v6.15c) <p>AND</p> <ul style="list-style-type: none"> ● PostgreSQL (for Expanse 2.2 only) OR Microsoft SQL Server AND ● IMO 2.0 (Intelligent Medical Objects)
<p>§170.315(f)(6) Antimicrobial Use and Resistance Reporting</p> <p>§170.315(g)(2) Automated measure calculation</p>	<ul style="list-style-type: none"> ● PostgreSQL (for Expanse 2.2 only) OR Microsoft SQL Server
<p>§170.315(g)(7) Application Access - Patient Selection</p> <p>§170.315(g)(9) Application Access - All Data Request</p> <p>§170.315(g)(10) Application Access - Standardized API for Patient and Population Services</p>	<p>For Ambulatory, Emergency Department Management</p> <ul style="list-style-type: none"> ● MEDITECH Expanse 2.2 Core HCIS (Version v2.2c) OR ● MEDITECH Expanse 2.1 Core HCIS (Version v2.1c) OR ● MEDITECH 6.1 Electronic Health Record Core HCIS (Version v6.15c)

STANDARDS UPDATES (INCLUDING STANDARDS VERSION ADVANCEMENT PROCESS (SVAP) AND UNITED STATES CORE DATA FOR INTEROPERABILITY (USCDI))

Standard (and version)	<p>Quality Reporting Document Architecture: Category I - Version 1.2</p> <p>Quality Reporting Document Architecture: Category III - Version 1.1</p>
------------------------	---

Updated certification criteria and associated product	170.315(c)(3) - Clinical quality measures (CQMs) — report
Health IT Module CHPL ID	<p>MEDITECH Expanse 2.2 Ambulatory v2.2c</p> <p>MEDITECH Expanse 2.2 Core HCIS v2.2c</p> <p>MEDITECH Expanse 2.2 Emergency Department Management v2.2c</p> <p>MEDITECH Expanse 2.2 Oncology v2.2c</p> <p>MEDITECH Expanse 2.1 Oncology v2.1c</p> <p>MEDITECH Expanse 2.1 Ambulatory v2.1c</p> <p>MEDITECH Expanse 2.1 Core HCIS v2.1c</p> <p>MEDITECH Expanse Emergency Department Management v2.1c</p> <p>MEDITECH 6.1 Electronic Health Record Core HCIS v6.15c</p> <p>MEDITECH 6.1 Oncology v6.15c</p> <p>MEDITECH 6.1 Emergency Department Management v6.15c</p> <p>MEDITECH 6.1 Ambulatory Electronic Health Record v6.15c</p>
Method used for standard update	Certification Attestation
Date of ONC -ACB notification	N/A
Date of customer notification (SVAP only)	N/A
Conformance measure	N/A
USCDI-updated certification criteria (and USCDI version)	N/A

Schedule of Key Milestones

MEDITECH, following change control approval procedures, connected to a number of predetermined customer directories or dedicated internal environments gathering data for a specific period each quarter beginning in January 2023 and throughout the year in order to capture metrics for each criterion. These statistics substantiate the demonstration of interoperability and functionality of our Certified Health IT in the care settings and scenarios for the 2023 test plan as described in the above scenarios. As criteria tests have been conducted, authorized MEDITECH representatives analyzed the result outcomes.

The execution of the testing process, capturing data on a quarterly basis, was completed in December 2023 for an analysis of success rates over a period of time for submission of reporting results due by February 2024.

Key Milestone	Care Setting	Timeframes
Initial development of the Real World Testing plans designed by platform combination.	Acute Ambulatory Emergency Oncology	August – October 2022
Development submission of reporting utilities to gather data for analysis.	Acute Ambulatory Emergency Oncology	August – October 2022
Submit final Real World Test plans to Drummond Group.	Acute Ambulatory Emergency Oncology	November 1, 2022
Post approved Real World Test Plan to external URL.		December 15, 2022
MEDITECH Initiated a collection of metrics for each group of criteria based on the reporting tools and utilities noted.	Acute Ambulatory	Quarterly – March, June, September, and December 2023
Met with designated testers and Certification group review for analysis of data collected.	Acute Ambulatory	March, June, September, and December 2023
Design Real World Testing Results Report	Acute Ambulatory	December 2023 - January 2024
Complete metric analysis and Real World	Acute	January 2024

Testing report completion.	Ambulatory	
Submit Real World Testing report to Drummond Group.	Acute Ambulatory	February 1, 2024

ATTESTATION

Authorized Representative Name: Geoffrey Smith
Authorized Representative Email: GSMITH@meditech.com
Authorized Representative Phone: 7781-774-4660
Date: January 17, 2024



Authorized Representative Signature:

MEDITECH Proprietary:
Statement for our customers: this document is intended for MEDITECH customers or their third-party vendors with a defined need. Please do not share this information outside of that scope.